

Model 428 Current Amplifier Quick Reference Guide

INTRODUCTION

This quick reference guide includes information on front panel operation for both the Model 428-MAN and the Model 428-PROG, as well as IEEE-488 operation information for the Model 428-PROG.

©1990, Keithley Instruments, Inc.
All rights reserved.
Instruments Division
Cleveland, Ohio U.S.A.
Document Number: 428-903-01 Rev. A

All Kelthley product names are trademarks of Kelthley instruments, Inc.

Other brand and product names are trademarks or registered trademarks of their respective holders.

TABLE OF CONTENTS

Safety Precautions	
Control Summary	5
Factory Default Conditions	
Display Messages	8
Test Connections	
Device-dependent Commands	11
Default/Alternate Output Word Formats	17
SRQ Mask and Serial Poll Byte	21

SAFETY PRECAUTIONS

- Before operation, ground the Model 428 through a properly-grounded power receptacle.
- Before servicing, disconnect the instrument from line power and all other equipment, and consult the Model 428 Instruction Manual.
- Do not touch any exposed terminals, cables, or wires while the instrument is turned on or connected to other test equipment.
- Do not exceed the maximum input levels as defined in the specifications (see Figure 1 of this guide and the Model 428 Instruction Manual).
- Exercise caution when a shock hazard is present. Voltage levels greater than 30V RMS, 42.4V peak are considered hazardous.
- Instrumentation and accessories should not be connected to humans.

CONTROL SUMMARY

DISPLAY INTENSITY: Selects normal/dim/off display.

LOCAL: Places unit in local and restores front panel key operation (428-PROG only).

MENU: Allows selection of firmware revision display, IEEE-488 primary address (428-PROG), autofilter on/off, save/recall configuration, and self-test.

SHIFT EXIT: Exits MENU.

ZERO CHECK: Allows check of offsets, and must be disabled to obtain normal output signal.

SHIFT CORRECT: Performs automatic zero correction to null instrument offsets.

SETUP GAIN: Use knob or cursor keys to set gain (10³V/A-10¹⁰V/A, with X10 gain off, 10⁴V/A-10¹¹V/A, with X10 gain on).

SETUP FILTER RISE TIME: Use knob or cursor keys to select filter rise time (10µsec-300msec),

SETUP CURRENT SUPPRESS: Use cursor keys to select suppress range and cursor position; use knob to adjust digit value (± 0.001 nA to ± 5 mA).

SETUP VOLTAGE BIAS: Use cursor keys to select digit; rotate knob to select digit value (± 2.5 mV to ± 5 V).

SHIFT AUTO: Performs automatic current suppression.

ENABLE keys: Enable/disable respective function (integral LED indicates when function is enabled).

FACTORY DEFAULT CONDITIONS

Mode	Default State
DISPLAY INTENSITY	Normal
CURRENT SUPPRESS	0.000mA, off
GAIN	10 ³ V/A
GAIN X10	Off
FILTER	Off
FILTER RISE TIME	10μsec
IEEE-488 Address*	22
VOLTAGE BIAS	0.000V, off
ZERO CHECK	On
AUTO FILTER	On .

^{*428-}PROG only

DISPLAY MESSAGES

Error Messages

Message	Туре	Description
CONFLICT*	Momentary	Suppress value too large for suppress
CORECT ERR	Latching	range Input offset too large for zero correct
IDDC.	Momentary	Invalid Device-dependent Command
IDDCO*	Momentary	Invalid Device-dependent Command Option
NO DFLTS	Latching	EEPROM checksum error during power up or device clear
NO REMOTE*	Momentary	X received while not in remote
OUT OF RNG	Momentary	Input current too large for auto suppress
OVERLOAD	Latching	Input or output over- load (message flashes while overload exists)
RAM ERROR	Latching	RAM error during self-
ROM ERROR	Latching	ROM error during self-
Z CHECK ON	Momentary	Auto suppress attempt with zero check on


^{*}IEEE-488 messages for Model 428-PROG only

Display Messages

Message*	Description
SHIFT CORRECTING SUPRESSING 1E03 V/A 10µsec 0.000mA 0.0000V REV A01** IEEE 22*** AUTOFILT Y AUTOFILT N DFLT OK DFLT SAVE DFLT RCL DFLT FCTRY SELFTEST N SELFTEST Y CHANGED NO CHANGE	SHIFT key pressed Unit performing zero correct Unit auto suppressing GAIN display FILTER RISE TIME display CURRENT SUPPRESS display VOLTAGE BIAS DISPLAY MENU software revision MENU lEEE-488 address MENU auto filter on MENU disable auto filter MENU no action on configuration MENU save configuration MENU recall saved configuration MENU recall saved configuration MENU restore factory defaults MENU do not perform self-test MENU perform self-test MENU term changed MENU text without change

- Numeric values depend on settings; factory defaults shown.
- ** Revision level may vary *** 428-PROG only

TEST CONNECTIONS

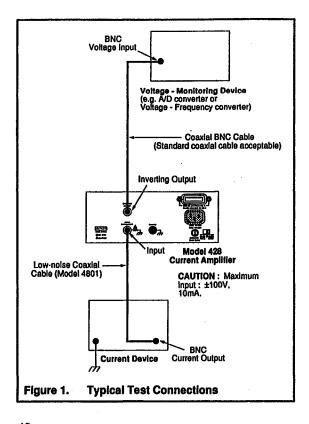

DEVICE-DEPENDENT COMMANDS

Display Intensity		
A0 A1 A2	Normal Dim Off	

Voltage E	Blas On/Off	
B0 B1	Turn voltage bias off Turn voltage bias on	

Zero Check/Zero Correct	
CO	Turn zero check off
C1	Turn zero check on
C2	Perform auto zero correct

Display		
DaaaaX Dx	Display string aaaa (10 max.) Return to normal display	

Hit Key	
H1	DISPLAY INTENSITY
H2	LOCAL
H3	SHIFT
H4	MENU
H5	ZERO CHECK
H6	SETUP GAIN
H7	SETUP FILTER RISE TIME
H8	SETUP CURRENT SUPPRESS
	SETUP CORRENT SUPPLESS SETUP VOLTAGE BIAS
H9	
H10	ENABLE GAIN X10
H11	ENABLE FILTER
H12	ENABLE CURRENT SUPPRESS
H13	ENABLE VOLTAGE BIAS
H14	◀
H15	
H16	Knob rotation counterclockwise
H17	Knob rotation clockwise

Self-test	
Jo	Test ROM and RAM only
J1	Test ROM, RAM, and display

EOI, Hold-off on X	
ко	Enable EOI, enable holdoff on X
K1	Disable EOI, enable holdoff on X
K2	Enable EOI, disable holdoff on X
КЗ	Disable EOI, disable holdoff on X

Save/rec	all
LO	Restore factory defaults and save
LO L1	Save configuration as power on
L2	Restore power-on conditions

SRQ Mask		
M1	Overload	
M2	Front panel key press	
M4	Not used	
M8	Not used	
M16	Ready for command	
M32	U1 error	

Suppression	
NO	Turn suppression off
N1	Turn suppression on
N2	Automatic suppress

Filter		
D0	Town Alban all	
P0	Turn filter off	
P1	Turn filter on	

Gain		
RO	10 ³ V/A gain	
R1	10°V/A gain	
R2	10 ³ V/A gain	
R3	10 ³ V/A gain	
R4	10⁴V/A gain	
R5	10⁵V/A gain	
R6	10 ⁶ V/A gain	
R7	10 ⁷ V/A gain	
R8	108V/A gain	
R9	10°V/A gain 10°V/A gain	
R10	1010V/A gain	

Suppress Range and Value	
S,0	Enable auto ranging
Sn,1	n = value, ±5nA range
Sn,2	n = value, ±50nA range
Sn,3	n = value, ±500nA range
Sn,4	n = value, ±5µA range
Sn,5	n = value, ±50μA range
Sn,6	n = value, ±500μA range
Sn,7	n = value, ±5mA range
Sn,8	IDDCO
Sn,9	IDDCO
Sn,10	Disable auto ranging

Rise Tim	0	
TO	10µsec	
T1	30µsec	
T2	100µsec	
T3	300µsec	
T4 T5	1msec	
T5	3msec	
T6	10msec	The state of the s
T7	30msec	
T8	100msec	
T9	300msec	4

Alternate Output (Status Words)		
UO	Send machine status word	
U1	Send error status word	
U2	Send blas value	
U3	Send total gain	
U4	Send model number, revision	

Voitage	Blas Value
Vn	-5 ≤ n ≤ +5V, 2.5mV resolution


X10 Gain On/Off		
wo	Turn X10 gain off	
W1	Turn X10 gain on	


Execute	
x	Execute DDCs previously sent


Terminator		
YO	<cr><lf></lf></cr>	
Y1	<lf><cr></cr></lf>	
Y2	<cr></cr>	
Y3	<lf></lf>	


Auto Filter	
Z0	Turn auto filter off
Z1	Turn auto filter on


DEFAULT/ALTERNATE OUTPUT WORD FORMATS

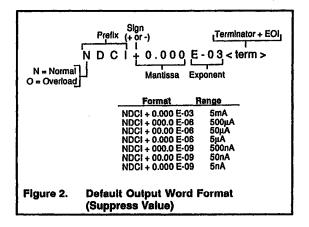


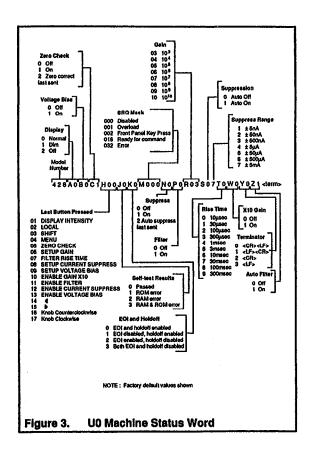

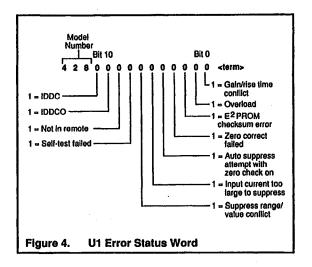


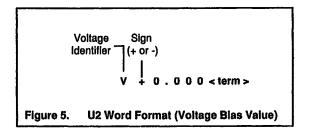

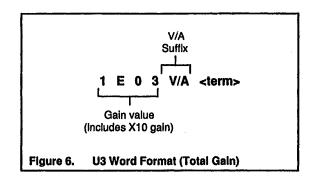

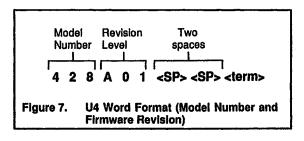

SRQ MASK AND SERIAL POLL BYTE

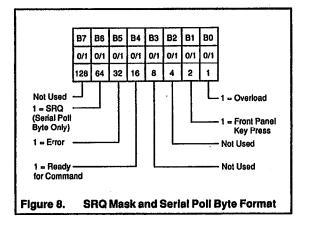

Specifications are subject to change without notice.

All Keithley trademarks and trade names are the property of Keithley Instruments, Inc. All other trademarks and trade names are the property of their respective companies.



Keithley Instruments, Inc.

28775 Aurora Road • Cleveland, Ohio 44139 • 440-248-0400 • Fax: 440-248-6168
1-888-KEITHLEY (534-8453) www.keithley.com

© Copyright 2000 Keithley Instruments, Inc. Printed in the U.S.A.